

Can disinfection robots reduce the risk of transmission of SARS-CoV-2 in healthcare and educational settings?

Kathrin Cresswell, Aziz Sheikh

Submitted to: Journal of Medical Internet Research
on: June 01, 2020

Disclaimer: © The authors. All rights reserved. This is a privileged document currently under peer-review/community review. Authors have provided JMIR Publications with an exclusive license to publish this preprint on its website for review purposes only. While the final peer-reviewed paper may be licensed under a CC BY license on publication, at this stage authors and publisher expressly prohibit redistribution of this draft paper other than for review purposes.

Table of Contents

Original Manuscript..... 4
Supplementary Files..... 10
 TOC/Feature image for homepages 11
 TOC/Feature image for homepage 0..... 12



Can disinfection robots reduce the risk of transmission of SARS-CoV-2 in healthcare and educational settings?

Kathrin Cresswell¹ BSc, MSc, PhD; Aziz Sheikh¹ OBE, FRSE, FMedSci

¹Usher Institute The University of Edinburgh Edinburgh GB

Corresponding Author:

Kathrin Cresswell BSc, MSc, PhD
Usher Institute
The University of Edinburgh
Teviot Place
Edinburgh
GB

Abstract

We here explore the opportunities and challenges surrounding the use of disinfection robots to reduce the risk of transmission of SARS-CoV-2 in healthcare and educational settings. Although there is some potential for deploying robots to help with manual cleaning, particularly if coupled with UV light and spraying of disinfectants, the evidence base is mixed and there needs to be work to establish and enhance the effectiveness of these robots in inactivating the virus.

(JMIR Preprints 01/06/2020:20896)

DOI: <https://doi.org/10.2196/preprints.20896>

Preprint Settings

1) Would you like to publish your submitted manuscript as preprint?

✓ **Please make my preprint PDF available to anyone at any time (recommended).**

Please make my preprint PDF available only to logged-in users; I understand that my title and abstract will remain visible to all users.

Only make the preprint title and abstract visible.

No, I do not wish to publish my submitted manuscript as a preprint.

2) If accepted for publication in a JMIR journal, would you like the PDF to be visible to the public?

✓ **Yes, please make my accepted manuscript PDF available to anyone at any time (Recommended).**

Yes, but please make my accepted manuscript PDF available only to logged-in users; I understand that the title and abstract will remain visible to all users.

Yes, but only make the title and abstract visible (see Important note, above). I understand that if I later pay to participate in <http://www.jmir.org/>

Original Manuscript



Can disinfection robots reduce the risk of transmission of SARS-CoV-2 in healthcare and educational settings?

Kathrin Cresswell, Chief Scientist Office Chancellor's Fellow, Director of Innovation, Usher Institute of Population Health Sciences and Informatics, The University of Edinburgh, UK

Aziz Sheikh, Professor of Primary Care Research & Development and Director, Usher Institute of Population Health Sciences and Informatics, The University of Edinburgh, UK

Correspondence to: K Cresswell, kathrin.cresswell@ed.ac.uk



SARS-CoV-2 can be transmitted through droplets and contact with contaminated surfaces.[1] In order to contain spread, there is a need for more regular and deeper cleaning of indoor surfaces, for example in schools, care homes and healthcare facilities. There is also a need to reduce human exposure to potentially contaminated surfaces. As a result, there is now an acceleration of interest of cleaning and disinfection robots in these settings.[2-4] Such robots are, for example, currently routinely cleaning the Hong Kong metro, and the Smart Field Hospital in Wuhan uses them in an attempt to reduce the spread of SARS-CoV-2.[5,6]

Existing disinfecting robots work through a combination of automated or semi-automated processes. They can clean or disinfect floors and surfaces, but increasingly focus on disinfecting whole rooms with increasingly complex distribution systems. These most commonly include machines drawing on ultraviolet C (or UVC) light, which work by altering DNA/RNA so that organisms cannot replicate, and vapour and fogging systems that essentially spray chemical disinfectants.

However, despite their increasing use and demand across settings, evidence of their effectiveness is mixed. There is no existing work exploring the effectiveness of disinfection robots in relation to SARS-CoV-2 and other viruses, and the evidence of the impact of UVC and vapour on Healthcare-Associated Infections (HAIs) and is also limited. In healthcare settings, both UVC light and chemical-based disinfection methods (most commonly hydrogen peroxide vapour) do not demonstrate any significant impact on reduced infection rates, although some studies have identified some positive trends and demonstrated a reduction in surface contamination.[7-9] Not surprisingly, UVC light and chemicals need to touch a surface to be effective and this may not always be the case – they have issues with shadows, may not reach all areas of concave surfaces, and their effectiveness reduces with distance.[10,11] This work is further complicated by a lack of evidence around how much contamination actually leads to infection and adverse patient outcomes, but there appears a general agreement that both techniques are most effective when combined with manual cleaning.[12] Studies investigating cleaning robots drawing on these techniques are very limited. The few existing investigations have found that cleaning robots drawing on UVC light and hydrogen peroxide can deliver some benefits in reducing microbial surface contamination, but only when combined with manual cleaning.[13,14] Study quality is relatively low for both applications with possible commercial biases.

Deploying the current generation of cleaning and disinfection robots in healthcare settings, care homes and schools is therefore unlikely to be of major benefit and there needs be work to establish and enhance the effectiveness of these robots in inactivating SARS-CoV-2. In addition to concerns around effectiveness, these devices are expensive at between \$30,000 and \$135,000 per unit and organisations need to train staff to deploy and control them.[13,15-17] Disinfectant chemicals and UVC light can also be dangerous to human health, so people typically need to leave while the robot cleans the room. This is particularly concerning for communal settings, but does not preclude the use of UVC light in enclosed empty spaces. Other factors to consider include disinfection time (some devices take a few hours per room), and issues with physical spaces and navigation (robots are not good at climbing stairs).[14,18]

Floor cleaning robots are likely to be cheaper units that can relatively easily and quickly be adapted (e.g. from other types of service robots) and that can focus on one aspect of the physical environment (i.e. the floor) whilst humans can work in parallel with them eliminating issues around disinfection time. There is therefore a need to catalyse development of floor cleaning robots that can regularly clean communal settings, particularly those with high risk of transmitting nosocomial infections. These devices can augment manual cleaning for instance through supporting an already stretched workforce and through reducing the risk of exposure for cleaning staff and those who work in these settings (e.g. doctors, nurses, assistants, teachers), particularly in the context of shortages of personal protective equipment (PPE). Some have noted issues with compliance of cleaning protocols promoting use of these robots and others have highlighted the importance of effective integration with existing routines and operations,[19,20] but this is unlikely to be a significant hurdle in times of

global need such as this. If the current generation cleaning and disinfectant robots are viewed as a panacea to reduce the spread of SARS-CoV-2, the resulting overreliance on their performance may jeopardise lives unnecessarily, but this is an area for urgent development that could help with lockdown exit strategies.

Funding: This work was funded by a Scottish Government Chief Scientist Research Grant. The views expressed are those of the authors.

Acknowledgements: We gratefully acknowledge all participants' time and input.

Conflict of interest: The authors declare no conflict of interest.




References

1. van Doremalen N, Bushmaker T, Morris DH, Holbrook MG, Gamble A, Williamson BN, Tamin A, Harcourt JL, Thornburg NJ, Gerber SI, Lloyd-Smith JO. Aerosol and surface stability of SARS-CoV-2 as compared with SARS-CoV-1. *New England Journal of Medicine*. 2020 Mar 17.
2. Robots: The Future of Cleaning? Available from: <https://servicesmag.org/online-digital-magazine/digital-archives/item/291-robots-the-future-of-cleaning> (last accessed: 15/04/2020).
3. Cleaning And Disinfection Robots Market growth is accelerating with a CAGR of 15.9%, during 2019-2025. Available from: https://www.marketwatch.com/press-release/cleaning-and-disinfection-robots-market-growth-is-accelerating-with-a-cagr-of-159-during-2019-2025-2019-09-09?mod=mw_quote_news (last accessed: 15/04/2020).
4. Hospital-Disinfecting Robots: Xenex Sees Surge In Orders As COVID-19 Pandemic Escalates. Available from: <https://news.crunchbase.com/news/hospital-disinfecting-robots-xenex-sees-surge-in-orders-as-covid-19-pandemic-escalates/> (last accessed: 15/04/2020).
5. Metro operator deploys cleaning robot to fight the coronavirus. Available from: <https://www.railwaygazette.com/technology-data-and-business/metro-operator-deploys-cleaning-robot-to-fight-the-coronavirus/55995.article> (last accessed: 15/04/2020).
6. Autonomous Robots Are Helping Kill Coronavirus in Hospitals. Available from: <https://spectrum.ieee.org/autoton/robotics/medical-robots/autonomous-robots-are-helping-kill-coronavirus-in-hospitals> (last accessed: 15/04/2020).
7. Anderson DJ, Chen LF, Weber DJ, Moehring RW, Lewis SS, Triplett PF, Blocker M, Becherer P, Schwab JC, Knelson LP, Lokhnygina Y. Enhanced terminal room disinfection and acquisition and infection caused by multidrug-resistant organisms and *Clostridium difficile* (the Benefits of Enhanced Terminal Room Disinfection study): a cluster-randomised, multicentre, crossover study. *The Lancet* 2017 Feb 25;389(10071):805-14.
8. Passaretti CL, Otter JA, Reich NG, Myers J, Shepard J, Ross T, Carroll KC, Lipsett P, Perl TM. An evaluation of environmental decontamination with hydrogen peroxide vapor for reducing the risk of patient acquisition of multidrug-resistant organisms. *Clinical infectious diseases*. 2013 Jan 1;56(1):27-35.
9. Non-Manual Ultraviolet Light Disinfection for Hospital Acquired Infections: A Review of Clinical Effectiveness and Guidelines. Available from: <https://www.ncbi.nlm.nih.gov/books/NBK544669/> (last accessed: 15/04/2020).
10. Yang JH, Wu UI, Tai HM, Sheng WH. Effectiveness of an ultraviolet-C disinfection system for reduction of healthcare-associated pathogens. *Journal of Microbiology, Immunology and Infection*. 2019 Jun 1;52(3):487-93.
11. Mana TS, Sitzlar B, Cadnum JL, Jencson AL, Koganti S, Donskey CJ. Evaluation of an automated room decontamination device using aerosolized peracetic acid. *American journal of infection control*. 2017 Mar 1;45(3):327-9.
12. Miller R, Simmons S, Dale C, Stachowiak J, Stibich M. Utilization and impact of a pulsed-xenon ultraviolet room disinfection system and multidisciplinary care team on *Clostridium difficile* in a long-term acute care facility. *American journal of infection control*. 2015 Dec 1;43(12):1350-3.
13. Doll M, Stevens M, Bearman G. Environmental cleaning and disinfection of patient areas. *International Journal of Infectious Diseases*. 2018 Feb 1;67:52-7.
14. Doll M, Morgan DJ, Anderson D, Bearman G. Touchless technologies for decontamination in the hospital: a review of hydrogen peroxide and UV devices. *Current infectious disease reports*. 2015 Sep 1;17(9):44.
15. UVC Disinfection Robot. Available from: [https://www.hipac.com.au/shop/uv-c-disinfection-](https://www.hipac.com.au/shop/uv-c-disinfection-robot)

- robot/index (last accessed: 15/04/2020).
16. Coronavirus: Robots use light beams to zap hospital viruses. Available from: <https://www.bbc.co.uk/news/business-51914722> (last accessed: 15/04/2020).
 17. Chinese company unveils \$40,000 hospital robot that uses a combination of UV light and liquid disinfectant spray to kill coronavirus pathogens. Available from: <https://www.dailymail.co.uk/sciencetech/article-8159921/Chinese-company-unveils-40-000-hospital-robot-disinfectants-against-coronavirus-pathogens.html> (last accessed: 15/04/2020).
 18. Hard Surface Disinfection System from Surfacide. Available from: <https://www.batesit.co.uk/helios-disinfection-system> (last accessed: 15/04/2020).
 19. Fleming M, Major Y, Gryskiewicz M, Fife J, Hassmer L, Masroor N, Cooper K, Doll M, Stevens M, Bearman G. Will Audit and Feedback Drive Compliance with UV Robot Disinfection?. *American Journal of Infection Control*. 2017 Jun 1;45(6):S51.
 20. Reduction of Healthcare Associated Infections through the use of Pulsed Xenon Ultraviolet Disinfection. Available from: https://www.sanimed.ro/upload_poze_documento/files/STUDII%20CLINICE.pdf (last accessed: 15/04/2020).

Supplementary Files

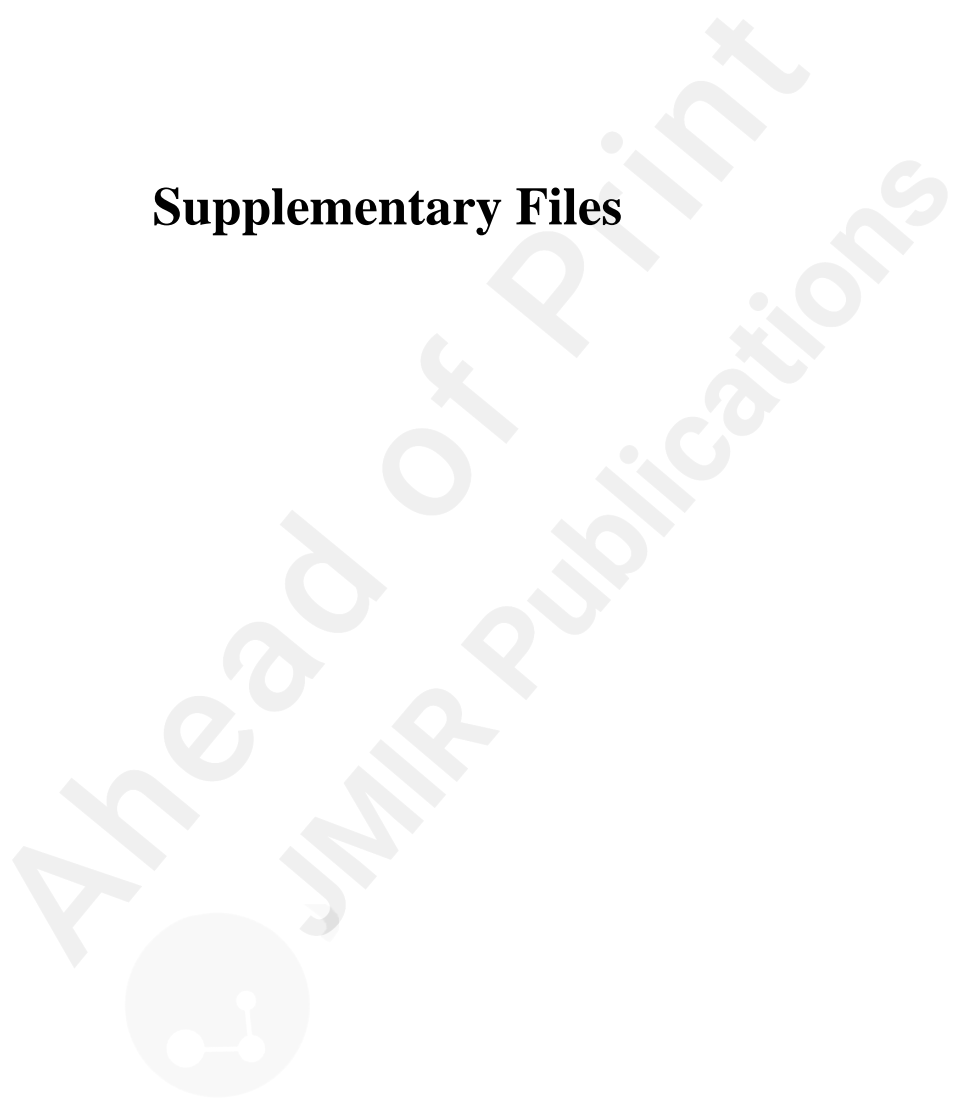

TOC/Feature image for homepages

Placeholder.

[PLACEHOLDER]